

INFECTION CONTROL



EDITORIAL

Risk Factors for Infection in Cardiac Surgery: Will the Real Culprit Please Stand Up?

Allen B. Kaiser, MD

ORIGINAL ARTICLES

Postoperative Wound Infections Following Cardiac Surgery: Significance of Contaminated Cases Performed in the Preceding 48 Hours

Malkanthie I. deSilva, MD; J. Peter Rissing, MD

Postoperative Infections Following Cardiac Surgery: Association with an Environmental Reservoir in a Cardiothoracic Intensive Care Unit

Peter C. Dandalides, MD; William A. Rutala, PhD; Felix A. Sarubbi, Jr., MD

Cost of Hepatitis B Prevention in Hospital Employees: Post-Exposure Prophylaxis

Bradford Kirkman-Liff, DrPH; Suzanne Dandoy, MD, MPH

Epidemic Keratoconjunctivitis: Report of an Outbreak in an Ophthalmology Practice and Recommendations for Prevention

James W. Buehler, MD; Robert J. Finton, MSPH;
Richard A. Goodman, MD, MPH; Keewhan Choi, PhD; John C. Hierholzer, PhD;
R. Keith Sikes, DVM, MPH; William R. Elsea, MD

Training of Personnel for Infection Control in Germany

Bernhard M. Thimm, DVM

Special Report: Recommendations for Decontaminating Manikins Used in Cardiopulmonary Resuscitation Training

Clinical Pharmacology of Antibiotics: Vancomycin— New Uses for an Old Drug

Sandra M. Norris, PharmD; Lynn Limon, RPh

Infection Control and Employee Health: A Cost-Effective Employee Health Program


William M. Valenti, MD

Infectious Waste Manager.™

Check the outstanding features of the infectious waste manager. Medical SafeTEC offers a variety of units, each incorporating these features, engineered to meet your infectious waste disposal needs. Sizes and features range from small, quiet waste stations for pharmacies, laboratories, or nursing stations to large central units with optional conveyor feed and automatic debris removal. Medical SafeTEC engineers will work with you to select the appropriate unit and implement a comprehensive infectious waste management system.

Infectious wastes in the destruction chamber are suspended in a steady flow of decontaminant solution. Interaction between the decontaminant and debris is accelerated by the hammermill action which reduces the waste to a fine, granular debris. All needles are broken and blunted. Plastics are shredded, and glass is returned to a sand-like material, safe from risk of puncture and infection.

Disposal equipment is totally safe in operation. Pneumatically-controlled, automatically-recycling feed hopper assures safe entry of materials into destruction chamber and prevents back spillage of materials during destruction process. Hopper sizes vary with each unit. Central units are designed to accept infectious waste collection containers to eliminate risk of sharps injuries and contact with infectious wastes. Conveyor feed of large bagged wastes is also available.

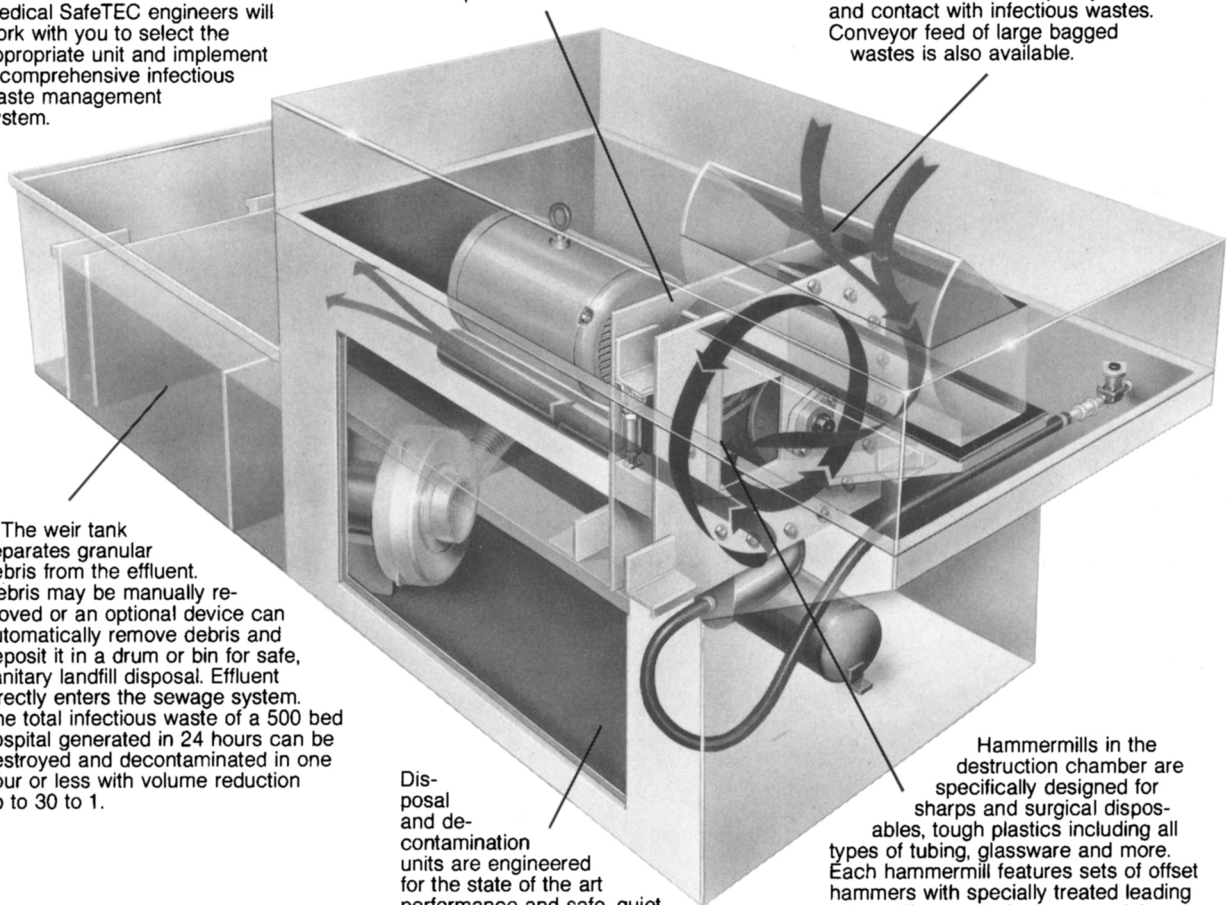

The weir tank separates granular debris from the effluent. Debris may be manually removed or an optional device can automatically remove debris and deposit it in a drum or bin for safe, sanitary landfill disposal. Effluent directly enters the sewage system. The total infectious waste of a 500 bed hospital generated in 24 hours can be destroyed and decontaminated in one hour or less with volume reduction up to 30 to 1.

Disposal and decontamination units are engineered for the state of the art performance and safe, quiet operation. Cabinetry is constructed of #16 GA type 304 stainless steel. The entire cabinet and weir tank operate in a negative air pressure to prevent the escape or build-up of infectious aerosols. Units are constructed of UL listed components and engineering specifications on each unit are available upon request.

Hammermills in the destruction chamber are specifically designed for sharps and surgical disposables, tough plastics including all types of tubing, glassware and more. Each hammermill features sets of offset hammers with specially treated leading edges. Tip speeds in some models exceed 240 miles per hour. A safety coupling transfers the power from the motor to the hammermill eliminating risk of motor overload.

For more information on complete infectious waste management systems contact Medical SafeTEC, Inc., 821 North Illinois, Indianapolis, Indiana 46204. 1-800-428-5008 or 317-263-3700.

Medical SafeTEC

Table of Contents

Editorial

- Risk Factors for Infection in Cardiac Surgery:
Will the Real Culprit Please Stand Up?** 369
Allen B. Kaiser, MD

Original Articles

- Postoperative Wound Infections Following Cardiac Surgery:
Significance of Contaminated Cases Performed in the Preceding 48 Hours** 371
Malkanthis I. deSilva, MD; J. Peter Rissing, MD
- Postoperative Infections Following Cardiac Surgery: Association with
an Environmental Reservoir in a Cardiothoracic Intensive Care Unit** 378
Peter C. Dandalides, MD; William A. Rutala, PhD; Felix A. Sarubbi, Jr., MD
- Cost of Hepatitis B Prevention in Hospital Employees:
Post-Exposure Prophylaxis** 385
Bradford Kirkman-Liff, DrPH; Suzanne Dandoy, MD, MPH
- Epidemic Keratoconjunctivitis: Report of an Outbreak in an
Ophthalmology Practice and Recommendations for Prevention** 390
James W. Buehler, MD; Robert J. Finton, MSPH;
Richard A. Goodman, MD, MPH; Keewhan Choi, PhD;
John C. Hierholzer, PhD; R. Keith Sikes, DVM, MPH; William R. Elsea, MD
- Training of Personnel for Infection Control in Germany** 395
Bernhard M. Thimm, DVM
- Special Report: Recommendations for Decontaminating Manikins Used in
Cardiopulmonary Resuscitation Training** 399
- Clinical Pharmacology of Antibiotics: Vancomycin—
New Uses for an Old Drug** 402
Sandra M. Norris, PharmD; Lynn Limon, RPh
- Infection Control and Employee Health: A Cost-Effective
Employee Health Program** 405
William M. Valenti, MD

Departments

- | | | | |
|--------------------------------|-----|-------------------------------|-----|
| Information for Authors | 364 | Calendar of Events | 409 |
| Letters to the Editor | 366 | Classified Marketplace | 412 |
| Book Reviews | 407 | | |

**The ideas and opinions expressed by contributing authors do not
necessarily reflect those of the editors or publisher.**

Publisher: *Infection Control* (ISSN-0195-9417) is published monthly by SLACK Incorporated, 6900 Grove Road, Thorofare, New Jersey 08086. Telephone: Thorofare (609) 848-1000.

Copyright 1984: All rights reserved. No part of this publication may be reproduced without written permission from the publisher.

Subscriptions: Subscription requests should be addressed to the publisher (except Japan). In Japan, contact Woodbell Scope Incorporated, 11-11, Shoto 2-chrome, Shibuya-Ku, Tokyo 150, Japan. Annual subscription price is: Individual: One year—\$35.00; Two years—\$50.00; Three years—\$65.00. Institutional: One year—\$50.00; Two years—\$65.00; Three years—\$80.00. All subscriptions, without exception, will start with the first issue published after the order is received. Back copies are available, but must be purchased separately. Cost per individual copy is \$5.00. Foreign subscribers add \$15.00 to regular rate: foreign orders, \$6.00.

Change of address: Notice should be sent to the publisher six weeks in advance of effective date. Include old and new addresses with zip codes. The publisher cannot accept responsibility for undelivered copies. Second-class postage is paid at Thorofare, New Jersey 08086. **Postmaster:** Form 3547 to SLACK Incorporated, 6900 Grove Road, Thorofare, NJ 08086.

As of Volume 1, Number 1, *Infection Control* is listed in *Index Medicus*, *Current Contents—Clinical Practice*, *Hospital Literature Index*, and *Cumulative Index to Nursing and Allied Health Literature*.

10 Reasons for Warming Up to a Cold Sterilant Wavicide-01[®]

1. The *least* expensive sterilant on the market.
2. Approved as a disinfectant, using a 1:4 dilution at room temperature.
3. Ready to use, Wavicide-01 works without an activator.
4. Sporocidal, as proven by AOAC test, at 25°C (10 hrs), 40°C (5 hrs) and 60°C (1 hr).
5. Approved for use in high-power ultrasonic cleaners.
6. Proven effective in continuous 28 day use and re-use with ultrasonic systems, even in the presence of organic matter.
7. Odorless when used as a disinfectant.
8. Will not yellow hands (some disinfectants do).
9. Will not fog or corrode fiberscopes.
10. Stable, long life, *balanced glutaraldehyde* formulation.

For literature or ordering information please contact:
Wave Energy Systems, Inc.
130 East 59 Street, 14 Floor
New York, NY 10022
(212) 593-3213

➔ **Wave Energy Systems Inc.**



Editorial Board

EDITOR

Richard P. Wenzel, MD
Charlottesville, Virginia

SENIOR ASSOCIATE EDITOR

William Schaffner, MD
Nashville, Tennessee

ASSOCIATE EDITORS

Sue Crow, RN, MSN
Shreveport, Louisiana

John E. McGowan, Jr., MD
Atlanta, Georgia

Dennis G. Maki, MD
Madison, Wisconsin



SLACK Incorporated
6900 Grove Road
Thorofare, New Jersey 08086

Publisher

Richard N. Roash

Managing Editor

Donna Carpenter

Consulting Editor

Eric Baloff

Assistant Editor

Jeanne M. Campo

Circulation Manager

Kevin J. Fenton

Advertising Manager

Melissa Warner

Advertising

Sales Representative

Wayne McCourt

Classified

Advertising Representative

Harriet E. Hampton

EDITORIAL ADVISORY BOARD

Robert C. Aber, MD
Hershey, Pennsylvania

Charles S. Bryan, MD
Columbia, South Carolina

John P. Burke, MD
Salt Lake City, Utah

Marie B. Coyle, PhD
Seattle, Washington

Richard E. Dixon, MD
Trenton, New Jersey

Harvey A. Elder, MD
Loma Linda, California

Peter C. Fuchs, MD, PhD
Portland, Oregon

Richard A. Garibaldi, MD
Farmington, Connecticut

Donald A. Goldmann, MD
Boston, Massachusetts

Dieter H.M. Gröschel, MD
Charlottesville, Virginia

Peter A. Gross, MD
Hackensack, New Jersey

Karen Hadley, RN, MPH
New Orleans, Louisiana

Cyrus C. Hopkins, MD
Boston, Massachusetts

Allen B. Kaiser, MD
Nashville, Tennessee

Harold Laufman, MD, PhD
New York, New York

William J. Ledger, MD
New York, New York

Barbara McArthur, RN, MS, PhD
Detroit, Michigan

Rob Roy MacGregor, MD
Philadelphia, Pennsylvania

C. Glen Mayhall, MD
Richmond, Virginia

Ronald Lee Nichols, MD
New Orleans, Louisiana

Harry C. Nottebart, Jr., JD, MD
Richmond, Virginia

Frank S. Rhame, MD
Minneapolis, Minnesota

William E. Scheckler, MD
Madison, Wisconsin

Robert J. Shannon, MSPH
Boston, Massachusetts

Walter E. Stamm, MD
Seattle, Washington

Charles W. Stratton, MD
Nashville, Tennessee

Timothy R. Townsend, MD
Baltimore, Maryland

William M. Valenti, MD
Rochester, New York

James Veazey, MD
Albany, New York

Kathy J. Wydra, RN
Geneva, New York

FOREIGN ADVISORY BOARD

Graham Ayliffe, MD, FRC Path.
Birmingham, England

Professor G. Berencsi
Szeged, Hungary

Professor Jaap Dankert
Groningen, Netherlands

Professor Dr. F. Daschner
Freiburg, West Germany

Lars O. Kallings, MD
Stockholm, Sweden

Professor W.B. Kędzia
Sieroca, Poland

Professor A.P. Krasilnikow
Minsk, USSR

Professor Dr. W. Marget
Munich, West Germany

Bertil Nyström, MD
Huddinge, Sweden

Ian Phillips, MA, MD, MRC Path.
London, England

Samuel Ponce de Leon, MD
Mexico City, Mexico

Hans Reber, MD
Basel, Switzerland

Professor Gerald Reybrouck
Leuven, Belgium

Manfred L. Rotter, MD, DipBact
Vienna, Austria

Theodore Sacks, MD
Jerusalem, Israel

Dr. Bernhard M. Thimm
Federal Republic of Germany

Professor Dr. med. H.P. Werner
Mainz, West Germany

Professor Dr. W. Weuffen
Greifswald, German Democratic Republic