

Volume 19, Number 5

October 2013

Microscopy AND Microanalysis




CAMBRIDGE
UNIVERSITY PRESS

ISSN 1431-9276

Living up to Life

Leica

MICROSYSTEMS

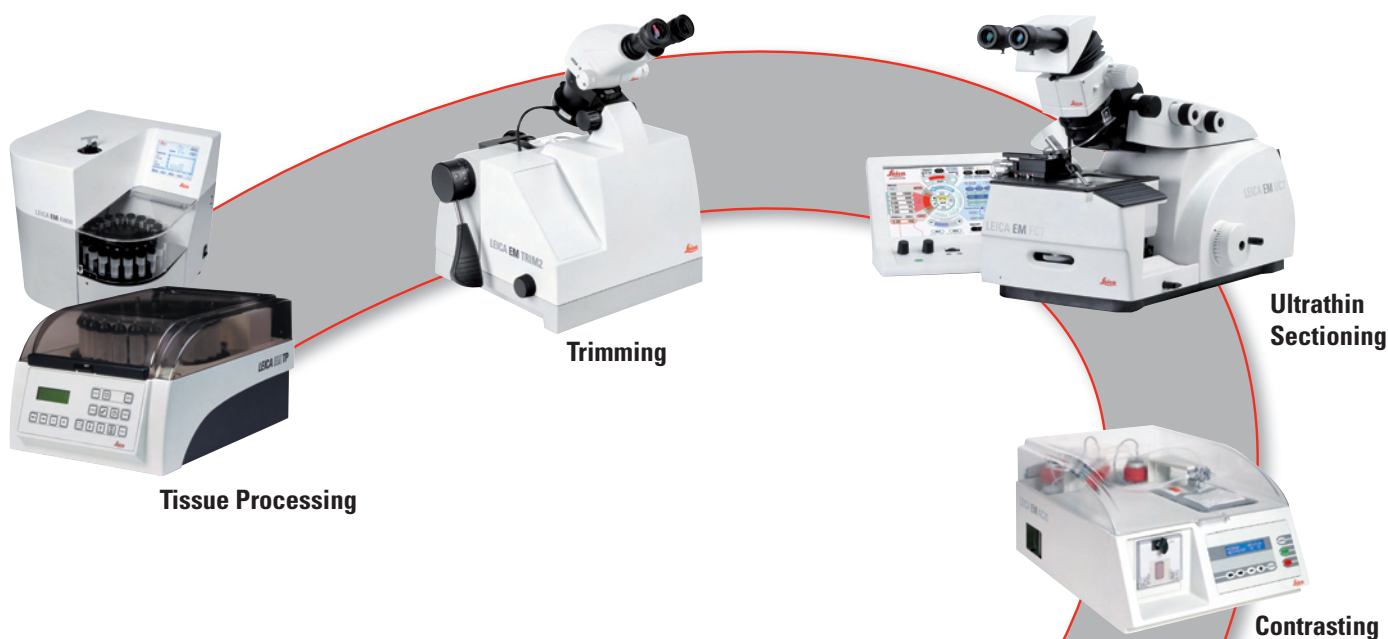

Visit www.leica-microsystems.com/em-promos to take advantage of Leica's current product promotions.

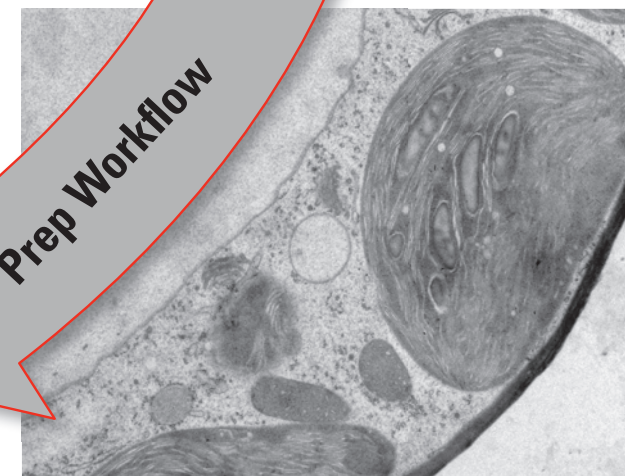


Image Analysis

Need Better EM Images?

Your Image Starts Here! Leica Microsystems' workflow solutions deliver excellent quality throughout every step of the sample preparation process. We offer the most comprehensive product portfolio for the preparation of biological, clinical, medical, and industrial samples for examination in the Electron Microscope (TEM – Transmission Electron Microscope and SEM – Scanning Electron Microscope), LM (Light Microscope), Confocal Microscope, and AFM (Atomic Force Microscope).

www.leica-microsystems.com

Microscopy AND Microanalysis

An International Journal for the Biological and Physical Sciences

THE OFFICIAL JOURNAL OF

MICROSCOPY SOCIETY OF AMERICA
MICROANALYSIS SOCIETY
MICROSCOPICAL SOCIETY OF CANADA /
SOCIÉTÉ DE MICROSCOPIE DU CANADA
MEXICAN MICROSCOPY SOCIETY
BRAZILIAN SOCIETY FOR MICROSCOPY AND MICROANALYSIS
VENEZUELAN SOCIETY OF ELECTRON MICROSCOPY
EUROPEAN MICROBEAM ANALYSIS SOCIETY
AUSTRALIAN MICROSCOPY AND MICROANALYSIS SOCIETY
PORTUGUESE SOCIETY FOR MICROSCOPY

PUBLISHED IN AFFILIATION WITH

ROYAL MICROSCOPICAL SOCIETY
GERMAN SOCIETY FOR ELECTRON MICROSCOPY
BELGIAN SOCIETY FOR MICROSCOPY
MICROSCOPY SOCIETY OF SOUTHERN AFRICA

Editor in Chief

Editor, Biological Applications

Robert L. Price
Cell and Developmental Biology and
Anatomy
University of South Carolina
Columbia, SC 29209
e-mail: Bob.Price@uscmed.sc.edu

Editor, Materials Applications

David J. Smith
Department of Physics
School of Materials
Arizona State University
Tempe, Arizona 85287-1504
e-mail: david.smith@asu.edu

Editor, Scanning Probe Microscopies

David Bell
School of Engineering & Applied
Sciences
Center for Nanoscale Systems
Harvard University
Cambridge, MA 02138
e-mail: dcb@seas.harvard.edu

Editor, Atom Probe

Thomas Kelly
Cameca Instruments, Inc.
A Business Unit of AMETEK, Inc.
Madison, WI 53711-4951
e-mail: Thomas.Kelly@ametec.com

Editor, Biological Applications

William A. Russin
Biological Imaging Facility
Department of Neurobiology
Northwestern University
Evanston, IL 60208
e-mail: w-russin@northwestern.edu

Editor, Biological Applications

Heide Schatten
Veterinary Pathobiology
University of Missouri-Columbia
Columbia, Missouri 65211-5030
e-mail: schattenh@missouri.edu

Editor, Microanalysis

John Mansfield
Electron Microbeam Analysis Lab
North Campus, 417 SRB
University of Michigan
Ann Arbor, MI 48109-2143
e-mail: jfmjfm@umich.edu

Editor, Correlative and Emerging Microscopy Applications

Vinayak P. Dravid
Materials Science and Engineering
Northwestern University
Evanston, Illinois 60208-3105
e-mail: v-dravid@northwestern.edu

Editor, Plant Biology Applications

Rosemary White
CSIRO Plant Industry
Canberra, ACT 2601, Australia
e-mail: rosemary.white@csiro.au

Special Issues and Reviews Editor

Jay Jerome
Vanderbilt University Medical Center
Nashville, TN 37232
e-mail: jay.jerome@vanderbilt.edu

Book Review Editor

Cynthia S. Goldsmith
Centers for Disease Control
Atlanta, GA 30333
e-mail: csg1@cdc.gov

M&M Program Guide Editor

Richard E. Edelmans
Miami University
Oxford, OH 45056
e-mail: edelmare@muohio.edu

Proceedings Editor

John Shields
University of Georgia
Athens, GA 30602
e-mail: jpshield@uga.edu

Editorial Board

Ralph Albrecht	<i>University of Wisconsin, Madison, Wisconsin</i>
Barry Carter	<i>University of Connecticut, Storrs, Connecticut</i>
Wah Chiu	<i>Baylor College of Medicine, Houston, Texas</i>
Niels de Jonge	<i>INM Institute for New Materials, Saarbrücken, Germany</i>
Alberto Diaspro	<i>University of Genoa, Italy</i>
Elizabeth Dickey	<i>Pennsylvania State University, University Park, Pennsylvania</i>
Alwyn Eades	<i>Lehigh University, Bethlehem, Pennsylvania</i>
Mark Ellisman	<i>University of California at San Diego, San Diego, California</i>
Pratibha Gai	<i>University of York, United Kingdom</i>
Marija Gajdardziska-Josifovska	<i>University of Wisconsin-Milwaukee, Milwaukee, Wisconsin</i>
Dale Johnson	<i>University of South Florida, Tampa, Florida</i>
Paul Kotula	<i>Sandia National Labs, Albuquerque, New Mexico</i>
William Landis	<i>University of Akron, Akron, Ohio</i>
Eric Lifshin	<i>SUNY at Albany, Albany, New York</i>
Charles Lyman	<i>Lehigh University, Bethlehem, Pennsylvania</i>
Dale Newbury	<i>National Institute of Standards and Technology, Gaithersburg, Maryland</i>
Jean-Paul Revel	<i>California Institute of Technology, Pasadena, California</i>
Conly Rieder	<i>Wadsworth Center, Albany, New York</i>
John Silcox	<i>Cornell University, Ithaca, New York</i>
Nan Yao	<i>Princeton University, Princeton, New Jersey</i>
Nestor Zaluzec	<i>Argonne National Laboratory, Argonne, Illinois</i>

Editorial Board Representatives from Affiliated Societies

Masashi Watanabe	<i>Lehigh University (MAS)</i>
Gautam Kumar Dey	<i>Bhabha Atomic Research Centre (EMSI)</i>
Gema Gonzalez	<i>Venezuelan Institute for Scientific Investigation (Venezuela)</i>
Michael Robertson	<i>Acadia University, Wolfville, Nova Scotia (Canada)</i>
Brendan Griffin	<i>University of Western Australia (AMMS)</i>
Guillermo Solorzano	<i>Pontificia Universidade Catolica, Rio de Janeiro (Brazil)</i>
Mike Matthews	<i>Institute for Transuranium Elements, Karlsruhe (EMAS)</i>
Miguel Yacamán	<i>Mexico Institute for Nuclear Research (Mexico)</i>
Henrique Almeida	<i>Universidade do Porto (Portugal)</i>

Founding Editor

Jean-Paul Revel	<i>California Institute of Technology, Pasadena, California</i>
-----------------	---

Previous Editors-in-Chief

Dale Johnson	<i>University of South Florida, Tampa, Florida</i>
Charles Lyman	<i>Lehigh University, Bethlehem, Pennsylvania</i>

This journal is part of the **Cambridge Journals Online** service. Access to online tables of contents and article abstracts is available to all researchers at no cost. Access to full-text articles online is provided to those with online subscription. Online subscriptions must be activated. Once your subscription is activated, free access to past, present, and forthcoming articles is available at:

Microscopy and Microanalysis website: journals.cambridge.org/MAM.

Instructions for authors submitting manuscripts may be found at journals.cambridge.org/MAM. Select "Further Information" then select "Instructions for Contributors." An abbreviated version of these instructions will be published in the first issue (February) of each volume.



NEW

SKYSCAN 1272: New generation of microtomographs from BRUKER MICROCT

EXCEPTIONAL PERFORMANCE BEYOND RESEARCHER'S IMAGINATIONS



free QR-reader app
is available in the AppStore

- Up to 209 Megapixel (14450 x 14450 pixels) in every virtual slice through objects
- More than 2600 such slices can be reconstructed after a single scan
- Due to phase-contrast enhancement, object details as small as 0.4 μ m can be detected
- Maximum scanning diameter - 75mm, integrated micropositioning stage
- Multithreaded CPU / GPU 3D reconstruction for single computer or cluster
- Possibility to scan samples during compression, tension, cooling or heating.
- 16-position sample changer with automatic adjustment of magnification and scanning protocol
- At the end of the scan the system can send you e-mail with a direct link to the scanning results
- The results can be exported to iPad or iPhone for 3D rendering by special software for mobiles

bruker-microct.com

microtomography

Innovation with Integrity

Microscopy and Microanalysis publishes original research papers dealing with a broad range of topics in microscopy and microanalysis. These include articles describing new techniques or instrumentation and their applications, as well as papers in which established methods of microscopy or microanalysis are applied to important problems in the fields of biology or materials science. Microscopy and microanalysis are defined here in a broad sense, and include all current and developing approaches to the imaging and analysis of microstructure. The criteria for acceptance of manuscripts are the originality and significance of the research, the quality of the microscopy or microanalysis involved, and the interest for our readership.

Four types of communications are published in the Journal. **Regular Articles** are of substantial length and describe the findings of an original research project that satisfies the aims and scope of the Journal, described above. **Review Articles** summarize the current status of an important area within the aims and scope of the Journal. **Letters to the Editor** usually contain comments on recent articles that have appeared in the Journal. **Book Reviews** are also published, but these are solicited only through the Book Review Editor.

Instructions for Contributors

Instructions for authors contributing manuscripts may be found at <http://mc.manuscriptcentral.com/mam> under "Resources: Instructions and Forms." Authors may also visit http://www.journals.cambridge.org/jid_MAM, select "Further Information," and then select "Instructions for Contributors." An abbreviated version of these instructions will be published in the first issue (February) of each volume.

Copyright Information

Submission of a manuscript implies: that the work described has not been published before (except in the form of an abstract or as part of a published lecture, review, or thesis); that it is not under consideration for publication elsewhere; that its publication has been approved by all coauthors, if any, as well as by the responsible authorities at the institute where the work has been carried out; that, if and when the manuscript is accepted for publication, the authors agree to automatic transfer of the copyright to the Microscopy Society of America; that the manuscript will not be published elsewhere in any language without the consent of the copyright holders; and that written permission of the copyright holder is obtained by the authors for material used from other copyrighted sources.

All articles published in this journal are protected by copyright, which covers the exclusive rights to reproduce and distribute the article (e.g., as offprints), as well as all translation rights. No material published in this journal may be reproduced photographically or stored on microfilm, in electronic data bases, video disks, etc., without first obtaining written permission from the publisher.

The use of general descriptive names, trade names, trademarks, etc., in this publication, even if not specifically identified, does not imply that these names lack protection by the relevant laws and regulation.

Authorization to photocopy items for internal or personal use, or the internal or personal use of specific clients, is granted by Cambridge University Press, provided that the appropriate fee is paid directly to Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, USA (Tel: (508) 750-8400), stating the ISSN (1431-9276), the volume, and the first and last page numbers of each article copied. The copyright owner's consent does not include copying for general distribution, promotion, new works, or resale. In these cases, specific written permission must first be obtained from the publisher.

Disclaimer

The Microscopy Society of America, the other societies stated, and Cambridge University Press cannot be held responsible for errors or for any consequences arising from the use of the information contained in this journal. The appearance of scientific reports and/or workshops, or any other material in *Microscopy and Microanalysis* does not constitute an endorsement or approval by The Microscopy Society of America of the findings, data, conclusions, recommendations, procedures, results, or any other aspect of the content of such articles. The appearance of advertising in *Microscopy and Microanalysis* does not constitute an endorsement or approval by The Microscopy Society of America of the quality or value of the products advertised or any of

the claims, data, conclusions, recommendations, procedures, results, or any other information included in the advertisements.

While the advice and information in this journal is believed to be true and accurate at the date of its going to press, neither the authors, the editors, nor the publisher can accept any legal responsibility for any errors or omissions that may be made.

Subscription Information

Microscopy and Microanalysis is published bimonthly in February, April, June, August, October, and December by Cambridge University Press. Two supplements (*Expo* and *Proceedings*) are published in June and August.

Society Rates: Members of the Microscopy Society of America should contact the MSA Business Office for all subscription inquiries: Microscopy Society of America, Hachero Hill, Inc., 11260 Roger Bacon Drive, Suite 402, Reston, VA 20190, Tel.: (703) 964-1240, Ext. 14, E-mail: nicoleguy@mindspring.com, URL: www.msa.microscopy.org. Members of other affiliated societies should contact their respective society business offices for all subscription inquiries.

Subscription Rates: Institutions print and electronic: US \$957.00 in the USA, Canada, and Mexico; UK £577.00 + VAT elsewhere. Institutions online only: US \$790.00 in the USA, Canada, and Mexico; UK £478.00 + VAT elsewhere. Institutions print only: US \$863.00 in the USA, Canada, and Mexico; UK £520.00 + VAT elsewhere. Individuals print and online: US \$359.00 in the USA, Canada, and Mexico; UK £218.00 + VAT elsewhere. Prices include postage and insurance.

USA, Canada, and Mexico: Subscribers in the USA, Canada, and Mexico should send their orders, with payment in US dollars or the equivalent value in Canadian dollars, to: Cambridge University Press, Customer Services Department (Journals), 100 Brook Hill Drive, West Nyack, NY 10994-2133, USA. Tel: (845) 353-7500. Fax: (845) 353-4141. Orders may be phoned direct (toll free): (800) 872-7423. E-mail: journals_subscriptions@cup.org.

Outside North America: Subscribers elsewhere should send their orders, with payment in sterling, to: Customer Services Department (Journals), Cambridge University Press, The Edinburgh Building, Shaftesbury Road, Cambridge, CB2 8RU, UK. Tel: +44 (0)1223 326070. Fax: +44 (0)1223 325150. E-mail: journals@cambridge.org

Change of address: Allow six weeks for all changes to become effective. All communications should include both old and new addresses (with postal codes) and should be accompanied by a mailing label from a recent issue. Society members should contact their respective society business offices to inform them of address changes.

Microform editions are available from: University Microfilms International, 300 North Zeeb Road, Ann Arbor, MI 48106, USA.

Editorial Office

Robert L. Price, Editor in Chief, Department of Cell and Developmental Biology and Anatomy, School of Medicine, University of South Carolina, 6439 Garner's Ferry Road, Bldg. 1 B-60, Columbia, SC 29209, USA; Tel: (803) 216-3824; Fax: (803) 733-3212; E-mail: Bob.Price@uscmed.sc.edu.

Office of Publication

Cambridge University Press, 32 Avenue of the Americas, New York, NY 10013-2473, USA; Tel: (212) 337-5000; Fax: (212) 337-5959.

Advertising Sales & Production

M.J. Mrvica Associates, Inc., 2 West Taunton Avenue, Berlin, NJ 08009, USA; Tel: (856) 768-9360; Fax: (856) 753-0064.

© 2013 by Microscopy Society of America. Printed in the United States on acid-free paper. Periodicals postage paid at New York, NY, and additional mailing offices. Return postage guaranteed. Postmaster: Send address changes in the U.S.A. and Canada to *Microscopy and Microanalysis*, Subscription Department, Cambridge University Press, 100 Brook Hill Drive, West Nyack, NY 10994-2133.



Cooling Stages

Recirculating Heaters
and Chillers

Sputter Coaters

SEM/TEM Carbon Coaters

Vacuum Evaporators

Glow Discharge Systems

RF Plasma Etchers/
Plasma Reactors

Critical Point Dryers

Freeze Dryers

Cryo-SEM Preparation
Systems

Vacuum Pumps & Accessories

Evaporation Supplies

and more...

well equipped...


Electron Microscopy Sciences is pleased to announce our new full line catalog, your comprehensive source for high-end Vacuum Equipment. EMS is committed to providing the highest quality products along with competitive pricing, prompt delivery and outstanding customer service.

and more...

Not just Vacuum Equipment, EMS also offers:

Laboratory Microwave Ovens • Automated Tissue Processors • Oscillating Tissue Slicers • Vibrating Microtomes • Rapid Immersion Freezers • Tissue Choppers • Desiccators and Desiccants • Centrifuges, Tubes, and Racks • Stirrers, Stirring Hotplates, and Digital Hotplates • Stirring Bars, Stirring Rods, and Hand Mixers • Vortex Mixers, Microplate Mixers, and Magnetic Stirrers • Tissue Rotators, Mixer Vortexes, and Rotator/Rockers • Dri Baths • Oven/Incubators • Cooling Chambers • Ultraviolet Lamps • Lab Jacks

For catalog requests, please visit our website at www.emsdiasum.com

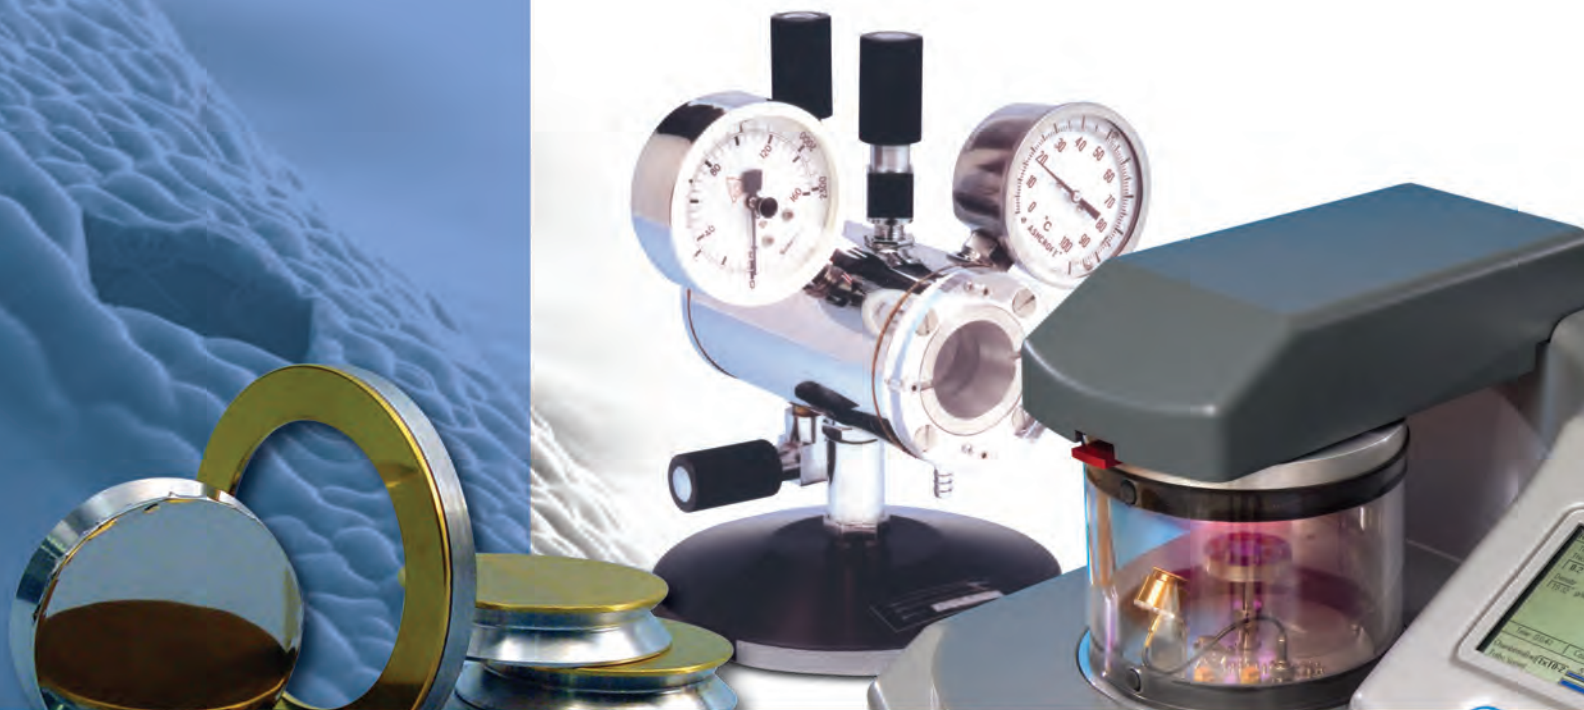

**Electron
Microscopy
Sciences**

Electron Microscopy Sciences
P.O. Box 550 • 1560 Industry Rd. • Hatfield, Pa 19440
Tel: (215) 412-8400 • Fax: (215) 412-8450
email: sgkck@aol.com • www.emsdiasum.com


FE SEM

7000 SERIES

CHOOSE THE PERFECT FE SEM FOR ALL YOU DO

- outstanding low kV/low vacuum performance
- high resolution imaging and nanoanalysis of structures, surface details, and magnetic samples
- high stable current with double condenser lens and aperture angle control lens
- multi-port chamber for in situ nanolab utility

Budget-conscious labs and leading-edge research centers will find the ultra versatility, performance, and support to be the perfect fit.

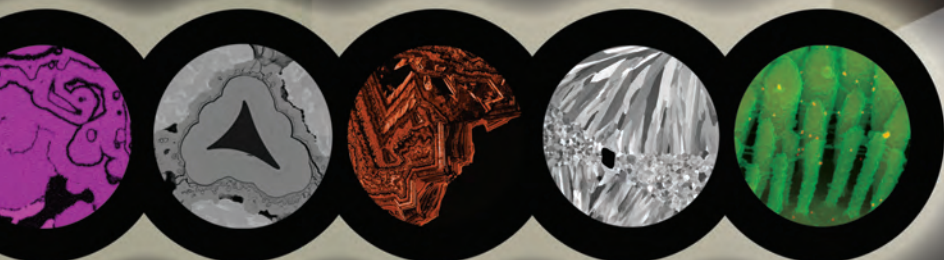

EDS

Backscatter

CL

Backscatter

Mixed SEBSE*

JEOL | www.jeolusa.com
salesinfo@jeol.com
978-535-5900

Solutions for Innovation

www.jeolusa.com/FESEM



* Courtesy of Dr. Artur Indzhyklian, Harvard Medical School

Microscopy AND Microanalysis

An International Journal for the Biological and Physical Sciences

Volume 19, Number 5

October 2013

PORTUGUESE SOCIETY FOR MICROSCOPY

Introduction: Portuguese Society for Microscopy 1109

A.P. Alves de Matos

Photobleaching/Photoblinking Differential Equation Model for Fluorescence
Microscopy Imaging 1110

J. Miguel Sanches and Isabel Rodrigues

Cellular Uptake Mechanisms of an Antitumor Ruthenium Compound:
The Endosomal/Lysosomal System as a Target for Anticancer
Metal-Based Drugs 1122

*Leonor Côte-Real, António P. Matos, Irina Alho, Tânia S. Morais, Ana Isabel Tomaz,
Maria Helena Garcia, Isabel Santos, Manuel P. Bicho, and Fernanda Marques*

Liver Alterations in Two Freshwater Fish Species (*Carassius auratus* and
Danio rerio) Following Exposure to Different TiO₂ Nanoparticle
Concentrations 1131

*Mário S. Diniz, António P. Alves de Matos, Joana Lourenço, Luísa Castro,
Isabel Peres, Elsa Mendonça, and Ana Picado*

Development and Evaluation of a Novel Topical Treatment for Acne
with Azelaic Acid-Loaded Nanoparticles 1141

*Catarina Pinto Reis, Ana Gomes, Patrícia Rijo, Sara Candeias, Pedro Pinto,
Marina Baptista, Nuno Martinho, and Lia Ascensão*

Structural Diversity of *Aspergillus* (Section *Nigri*) Spores 1151

Marta Filipa Simões, Cledir Santos, and Nelson Lima

Exploring the Contribution of Mycobacteria Characteristics in Their
Interaction with Human Macrophages 1159

*Carla Silva, Joao Perdigão, Elsa Alverca, António P. Alves de Matos,
Patricia A. Carvalho, Isabel Portugal, and Luisa Jordao*

Texture Indicators for Segmentation of Polyomavirus Particles in
Transmission Electron Microscopy Images 1170


Maria C. Proença, José F.M. Nunes, and António P.A. de Matos

Iridovirus-Like Viruses in Erythrocytes of Lacertids from Portugal 1183

*António P. Alves de Matos, M. Filomena Caeiro, Filipa F. Vale, Eduardo Crespo,
and Ilan Paperna*

Structure and Growth of Sialoliths: Computed Microtomography and
Electron Microscopy Investigation of 30 Specimens 1190

*Pedro Nolasco, Ana J. Anjos, João M. Aquino Marques, Fernando Cabrita,
Eduardo Carreiro da Costa, António Maurício, Manuel F.C. Pereira,
António P. Alves de Matos, and Patricia A. Carvalho*

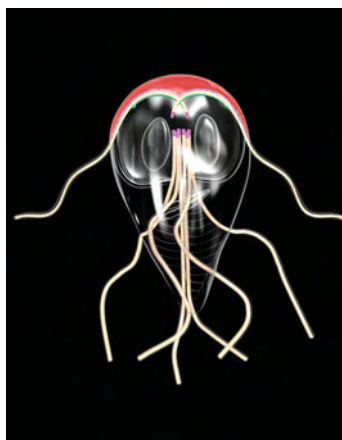

On the Cover: Model for anterior flagella complex of *Giardia duodenalis*. For further information see Maia-Brigagão et al., pp. 1374–1376.

Microscopy and Microanalysis website: <http://www.journals.cambridge.org/MAM>
Indexed in Chemical Abstracts, Current Contents, BIOSIS, and MEDLINE (PubMed)

HOLZ Rings in EBSD Patterns of the UFeB ₄ Compound: Association with a Random Distribution of Planar Defects	1204
<i>Marta Dias, Patrícia Almeida Carvalho, Isabel Cordeiro dos Santos, Olivier Tougait, Ladislav Havela, and António Pereira Gonçalves</i>	
Electron Diffraction of ThMn ₁₂ /Th ₂ Zn ₁₇ -Type Structures in the Nd-Fe-Ti System	1211
<i>Daniela Nunes, António P. Gonçalves, and Patricia A. Carvalho</i>	
Intrinsically Fluorescent Silica Nanocontainers: A Promising Theranostic Platform	1216
<i>Ana S. Rodrigues, Tânia Ribeiro, Fábio Fernandes, José Paulo S. Farinha, and Carlos Baleizão</i>	
Microstructural Characterization of Concrete Prepared with Recycled Aggregates	1222
<i>Mafalda Guedes, Luís Evangelista, Jorge de Brito, and Alberto C. Ferro</i>	
Susceptibility of Limestone Petrographic Features to Salt Weathering: A Scanning Electron Microscopy Study	1231
<i>Carlos Alves, Carlos Figueiredo, António Maurício, and Luís Aires-Barros</i>	
Scanning Electron Microscopy Studies of Neoformations on Stony Materials of Modern Building Works	1241
<i>Carlos Alves</i>	
Multifocus Optical Microscopy Applied to the Study of Archaeological Metals	1248
<i>Elin Figueiredo, Rui J.C. Silva, M. Fátima Araújo, and Francisco M. Braz Fernandes</i>	
TECHNIQUES AND SOFTWARE DEVELOPMENT	
Dynamical Electron Backscatter Diffraction Patterns. Part I: Pattern Simulations	1255
<i>Patrick G. Callahan and Marc De Graef</i>	
Phase Classification by Mean Shift Clustering of Multispectral Materials Images	1266
<i>Diego Schmaedeck Martins, Victor M. Galván Josa, Gustavo Castellano, and José A.T. Borges da Costa</i>	
The Determination of Rotation Axis in the Rotation Electron Diffraction Technique	1276
<i>Mika Buxhuku, Vidar Hansen, Peter Oleyniko, and Jon Gjønnes</i>	
Rapid and Accurate Analysis of an X-Ray Fluorescence Microscopy Data Set through Gaussian Mixture-Based Soft Clustering Methods	1281
<i>Jesse Ward, Rebecca Marvin, Thomas O'Halloran, Chris Jacobsen, and Stefan Vogt</i>	
A Scanning Transmission Electron Microscopy Approach to Analyzing Large Volumes of Tissue to Detect Nanoparticles	1290
<i>Paul J. Kempen, Avnesh S. Thakor, Cristina Zavaleta, Sanjiv S. Gambhir, and Robert Sinclair</i>	
MATERIALS APPLICATIONS	
The Origin of Long-Period Lattice Spacings Observed in Iron-Carbide Nanowires Encapsulated by Multiwall Carbon Nanotubes	1298
<i>Filippo S. Boi, Gavin Mountjoy, Zofia Luklinska, Liam Spillane, Lisa S. Karlsson, Rory M. Wilson, Anna Corrias, and Mark Baxendale</i>	
Complex Defect in Pyrite and Its Structure Model Derived from Geometric Phase Analysis	1303
<i>Péter Németh, István Dódon, Mihály Pósfai, and Peter R. Buseck</i>	
Phases in the Al-Corner of the Al-Mn-Be System	1308
<i>Franc Zupanič, Boštjan Markoli, Iztok Naglič, Tobias Weingärtner, Anton Meden, and Tonica Bončina</i>	
Water Exclusion Layers Probed by Depth Scan Confocal Raman Microscopy	1317
<i>Omar Teschke, Luiz O. Bonugli, and Marcus V.P. dos Santos</i>	

BIOLOGICAL APPLICATIONS

- Oligomers Modulate Interfibril Branching and Mass Transport Properties of Collagen Matrices 1323
Catherine F. Whittington, Eric Brandner, Ka Yaw Teo, Bumsoo Han, Eric Nauman, and Sherry L. Voytik-Harbin
- Structural and Biomechanical Effects of Photooxidative Collagen Cross-Linking with Photosensitizer Riboflavin and 370 nm UVA Light on Human Corneoscleral Tissues 1334
Samjin Choi, Jae-Ho Shin, Youjin Cheong, Kyung-Hyun Jin, and Hun-Kuk Park
- Atomic Force Microscopy Characterization of the External Cortical Bone Surface in Young and Elderly Women: Potential Nanostructural Traces of Periosteal Bone Apposition During Aging 1341
Petar Milovanovic, Marija Djuric, Olivera Neskovic, Danijela Djonc, Jelena Potocnik, Slobodan Nikolic, Milovan Stoiljkovic, Vladimir Zivkovic, and Zlatko Rakocevic
- Biodegradation Process of α -Tricalcium Phosphate and α -Tricalcium Phosphate Solid Solution Bioceramics *In Vivo*: A Comparative Study 1350
Piedad N. de Aza, Zofia B. Luklinska, Jose E. Mate-Sanchez de Val, and Jose L. Calvo-Guirado
- Imaging of *Xenopus laevis* Oocyte Plasma Membrane in Physiological-Like Conditions by Atomic Force Microscopy 1358
Massimo Santacroce, Federica Daniele, Andrea Cremona, Diletta Scaccabarozzi, Michela Castagna, and Francesco Orsini
- Clathrin Heavy Chain 1 is Required for Spindle Assembly and Chromosome Congression in Mouse Oocytes 1364
Jie Zhao, Lu Wang, Hong-Xia Zhou, Li Liu, Angeleem Lu, Guang-Peng Li, Heide Schatten, and Cheng-Guang Liang
- New Associated Structures of the Anterior Flagella of *Giardia duodenalis* 1374
Claudia Maia-Brigagão, Ana Paula Rocha Gadelha, and Wanderley de Souza



Systems smart enough to help you reach the summit.

At EDAX we understand how you see the world. Tackle your next materials challenge with one of our **TEAM™ Trident Analysis Systems**, the industry's most comprehensive microanalysis solution.

- EDS, EBSD and WDS seamlessly integrated with a single user interface.
- Built-in Smart Features facilitate set-up, guide analysis and automate reporting.
- Proven algorithms guarantee quality results.
- Streamlined workflows drive productivity with industry-best results in three mouse clicks.

Power your next insight with EDAX.



AMETEK®
MATERIALS ANALYSIS DIVISION

[edax.com](https://www.edax.com)

EDAX®
Smart Insight

The moment "I think" becomes "I know".
This is the moment we work for.

// TECHNOLOGY
MADE BY CARL ZEISS

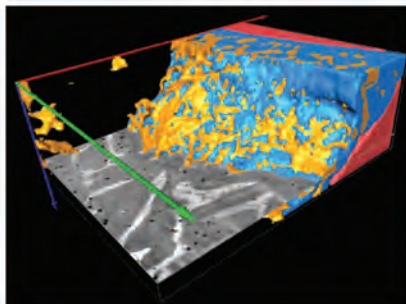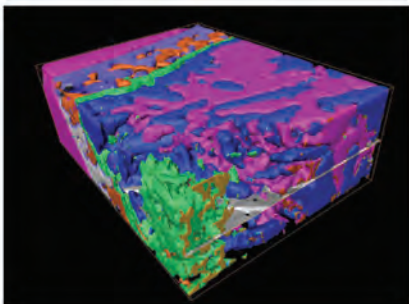

Three-dimensional ED_S microanalysis by FIB-SEM characterizing complex metal alloy phases

ZEISS is the world's microscopy leader in three-dimensional imaging. Visit us at booth #1008 at M&M 2013 and test our different solutions that can create precise, three-dimensional representations of samples ranging in size from millimeters to nanometers.

www.zeiss.com/m&m








We make it visible.



High Definition Digital
TEM Cameras with
1 to 16 Megapixels

- AMT SOLUTIONS
- Life Science Cameras
- Material Science Cameras
- Easy To Use Software
- Reliability and Services
- TEM Integration
- Extensive Support



3 Electronics Avenue, Danvers, MA 01923 • Phone: 978.774.5550 • www.amtimaging.com

FEI is changing the world of TEM




...so you can change yours.

See the new lineup of TEM instruments:
FEI.com/TEMbyFEI

#TEMbyFEI




Explore. Discover. Resolve.




PELCO BioWave® Pro

Fast, Low Temperature
Microwave Tissue Processing



- Rapid specimen turnaround
- Low temperature environment
- Programmable processing
- Consistent quality results



Application kits for paraffin processing, decalcification, confocal, light and electron microscopy available.






TED PELLA, INC.
Microscopy Products for Science and Industry

www.tedpella.com sales@tedpella.com 800.237.3526

SIA

1 TO 50 MEGAPIXELS live and slow scan
MAGNIFICATION FACTOR OF 1 on bottom mounted cameras
DIFFRACTION BEAM STOP on side mounted cameras

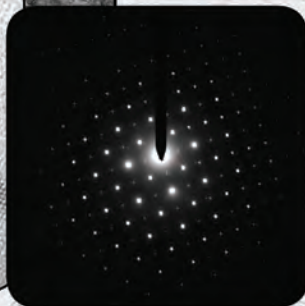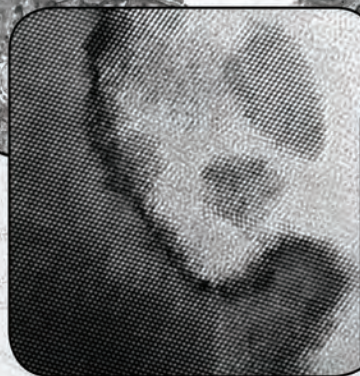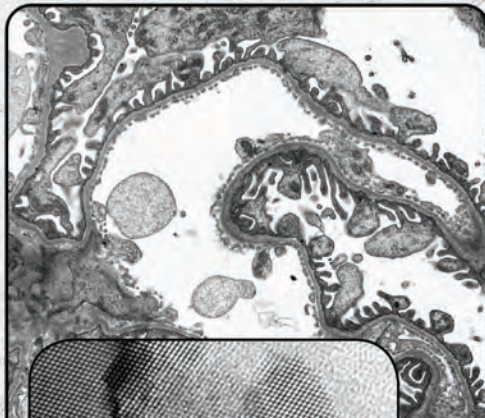

Affordable TEM camera systems for research, education, healthcare, and industry since 2001

Scientific Instruments and Applications
2773 Heath Lane • Duluth, GA 30096
(770) 232 7785 • www.sia-cam.com

The SPI Supplies Family of Instruments



Excellence in sample preparation
just a click away... 2spi.com

Your results will never be better than your sample preparation. See how SPI Supplies can help you deliver the highest quality results for all your SEM/EDS, TEM and FESEM applications.

1. Osmium Plasma Coaters for FESEM Applications
2. SPI-MODULE™ Sputter/Carbon Coater Module
3. Gentle Mill™ Ion Milling System
4. Plasma Prep™ III Solid State Plasma Cleaner for cleaning TEM holders

5. Plasma Prep™ X Parallel Plate Plasma Etcher
6. Plasma Prep™ III Plasma Etcher with PPIII Process Controller
7. Vacu Prep™ II Turbo Pump Evaporation System
8. SPI-DRY™ Critical Point Dryer
9. Precision Spin Coater Spin coater






SPI Supplies Division of **STRUCTURE PROBE, Inc.**

P.O. Box 656 • West Chester, PA 19381-0656 USA
Phone: 1-610-436-5400 • 1-800-2424-SPI (USA and Canada) • Fax: 1-610-436-5755 • 2spi.com • E-mail: sales@2spi.com



**the highest quality...
the most precise sectioning...
incomparable durability**

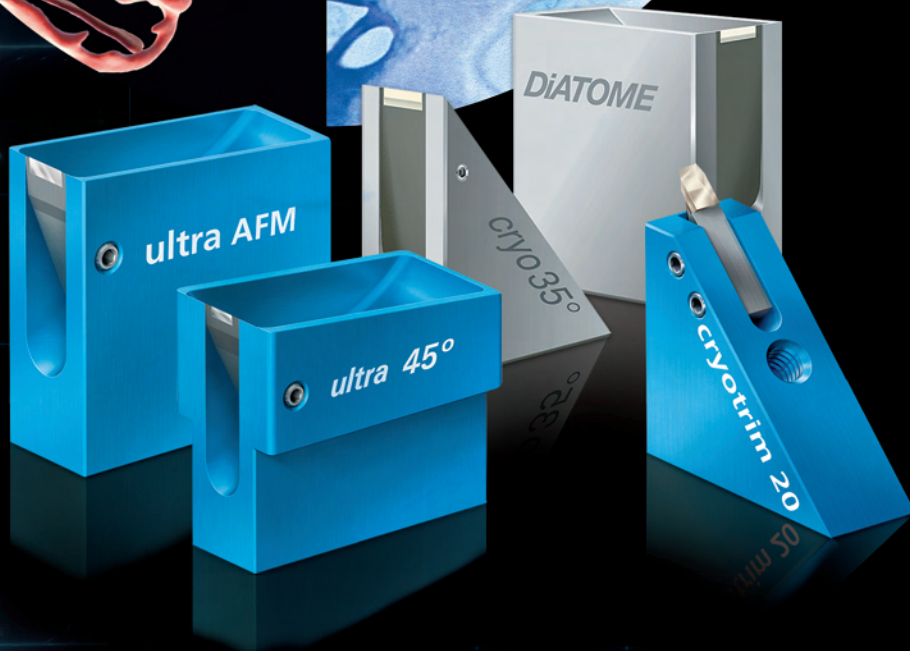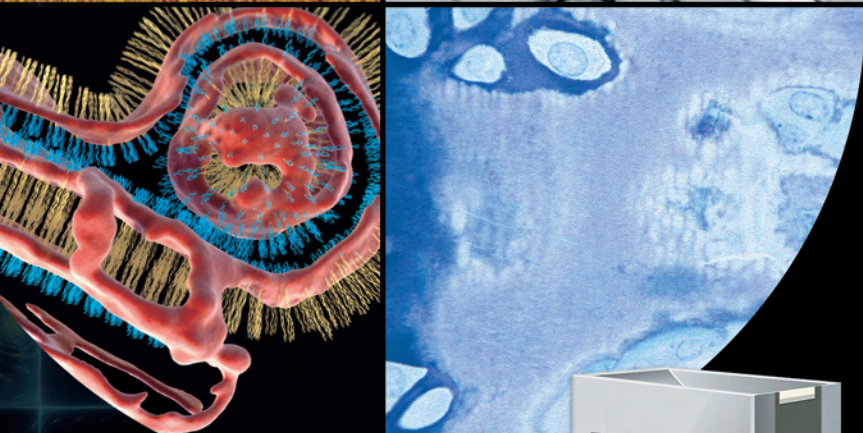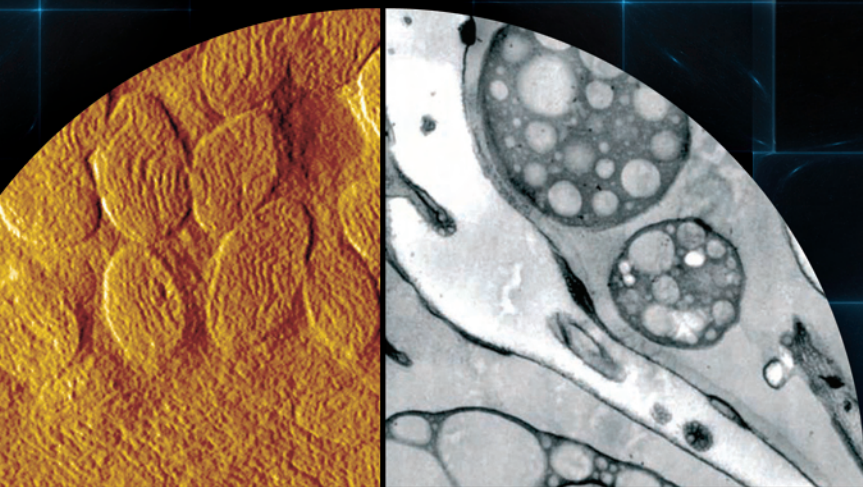

Free Customer Service

Sectioning tests with biological and material research specimens of all kinds. We send you the sections along with the surfaced sample, a report on the results obtained and a recommendation of a suitable knife. Complete discretion when working with proprietary samples.

Re-sharpening and Reworking Service

A re-sharpened Diatome diamond knife demonstrates the same high quality as a new knife. Even knives purchased in previous years can continue to be re-sharpened. The knives can be reworked into another type of knife for no extra charge, e.g. ultra to cryo or 45° to 35°.

Exchange Service

Whenever you exchange a knife we offer you a new Diatome knife at an advantageous price.

40 years of development,
manufacturing, and
customer service

DiATOME
diamond knives

ultra 45° • cryo • histo • ultra 35° • STATIC LINE II
cryo-P • cryo immuno • ultra sonic
cryotrim 45 and 25 ultra • AFM & cryo AFM • cryo 25°

DiATOME US • P.O. Box 550 • 1560 Industry Rd. • Hatfield, Pa 19440

Tel: (215) 412-8390 • Fax: (215) 412-8450 • email: sgkcck@aol.com • www.emsdiasum.com