


Volume 19, Number 1

February 2013

# Microscopy AND Microanalysis

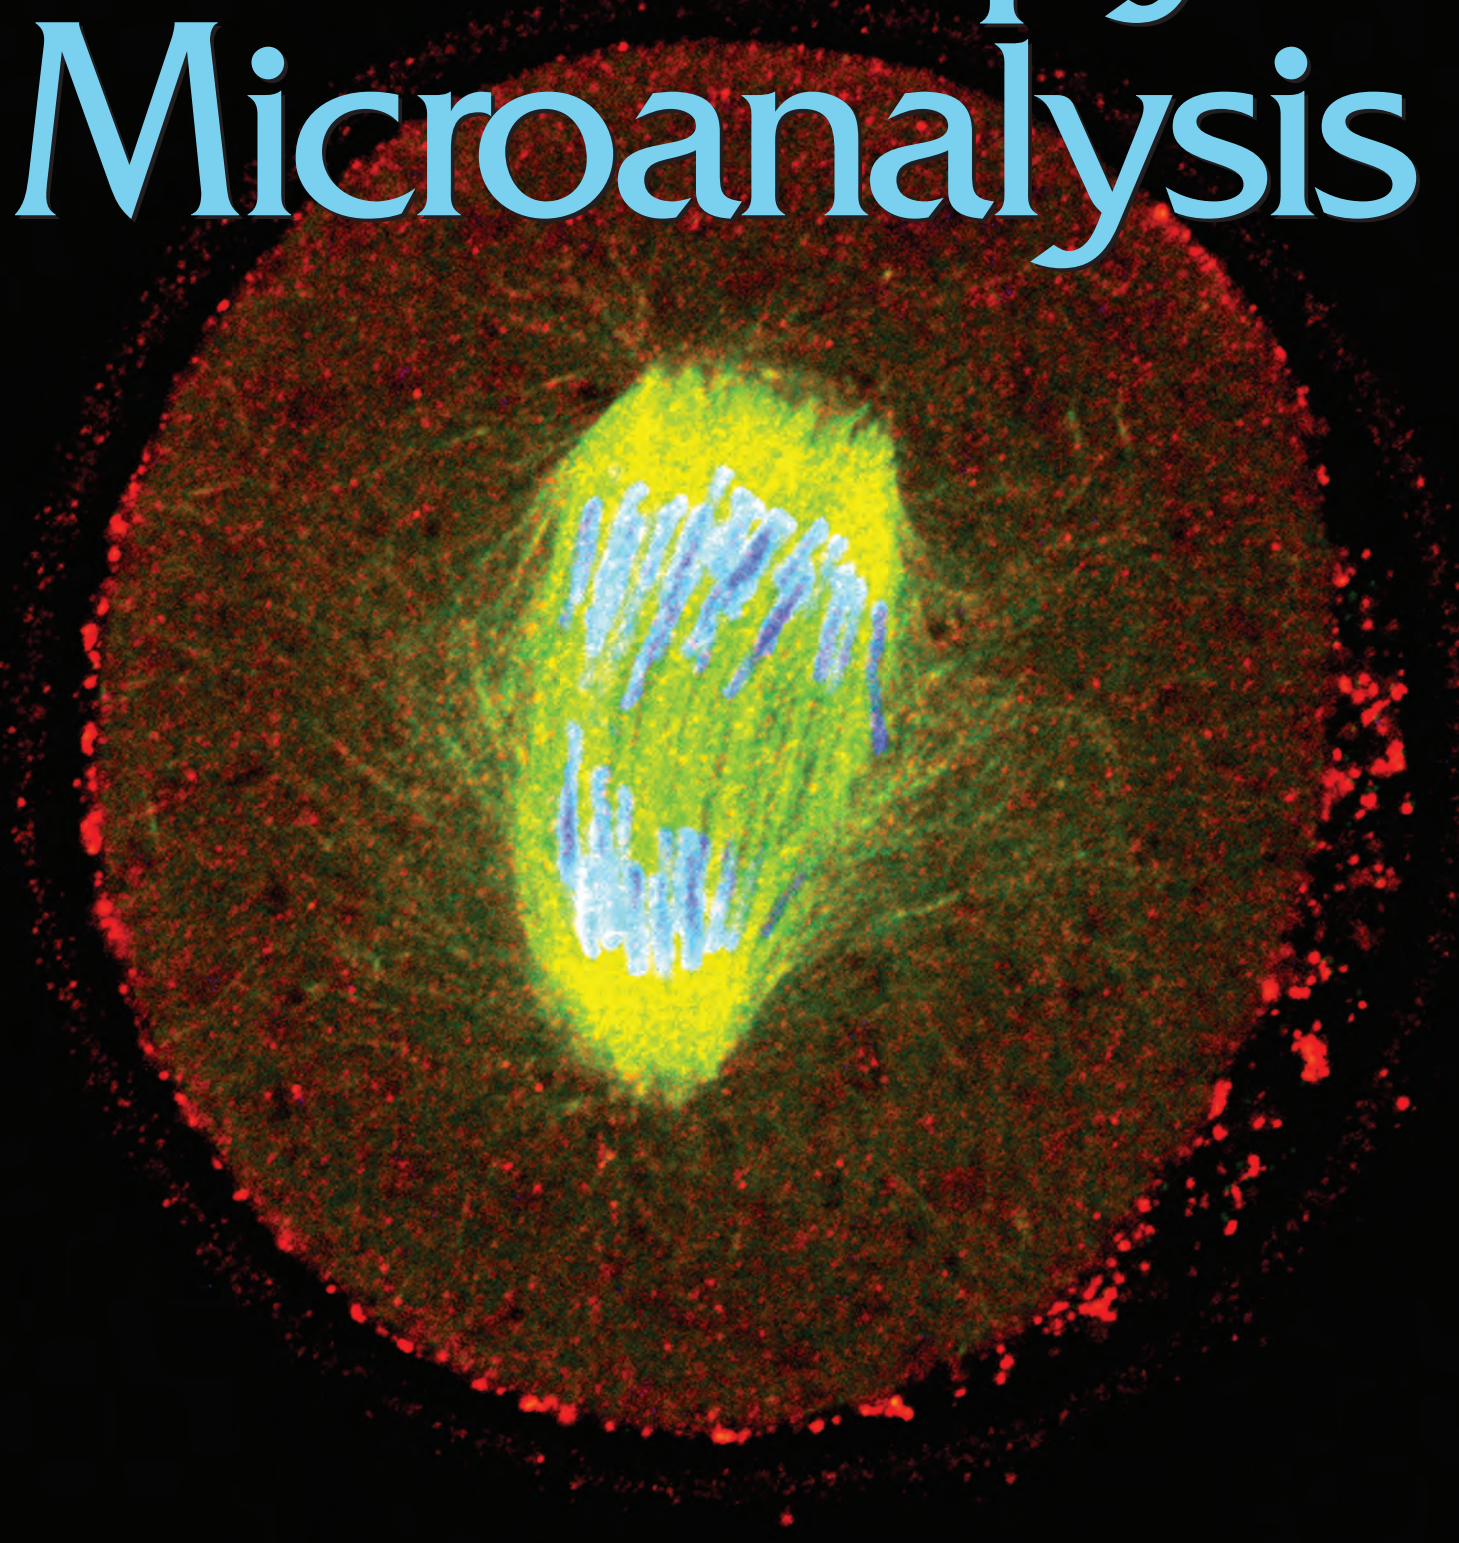


CAMBRIDGE  
UNIVERSITY PRESS

ISSN 1431-9276

Living up to Life

**Leica**  
MICROSYSTEMS

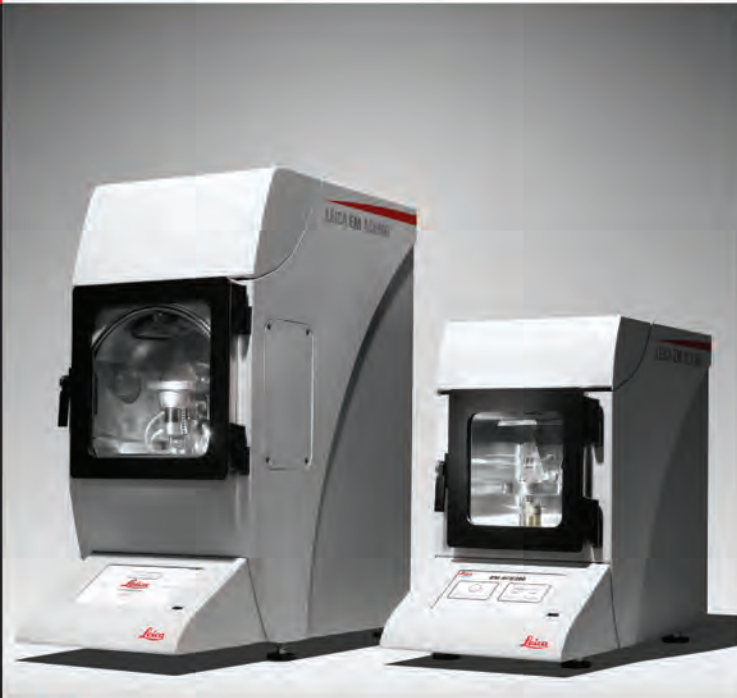

**NEW!** Leica EM ACE Coaters



Courtesy of Mag. D Gruber, Core Facility of Cell Imaging and Ultrastructure Research, University of Vienna, Austria

## Leica Microsystems Announces the Release of the **NEW** Leica EM ACE Coaters

The ultimate quality of a microscopic image comes from high-quality sample preparation. Leica Microsystems has a full range of innovative instrumentation to deliver perfect preparation for all sample materials.

**NEW! Leica EM ACE:** Coating systems for the preparation of samples for the Scanning Electron Microscope (SEM), Transmission Electron Microscope (TEM) and the Field Emission Scanning Electron Microscope (FE-SEM).

- Fully Automated, One-touch Coating Systems **for convenience**
- Low Vacuum or High Vacuum with Optional Cryo **for flexibility**
- Small Footprint **for more workspace**



Visit [www.leica-microsystems.com/mm\\_ace](http://www.leica-microsystems.com/mm_ace) to see Leica Microsystems' latest sample preparation solutions!

# Microscopy AND Microanalysis

**An International Journal for the Biological and Physical Sciences**

THE OFFICIAL JOURNAL OF

MICROSCOPY SOCIETY OF AMERICA  
MICROANALYSIS SOCIETY  
MICROSCOPICAL SOCIETY OF CANADA /  
SOCIÉTÉ DE MICROSCOPIE DU CANADA  
MEXICAN MICROSCOPY SOCIETY  
BRAZILIAN SOCIETY FOR MICROSCOPY AND MICROANALYSIS  
VENEZUELAN SOCIETY OF ELECTRON MICROSCOPY  
EUROPEAN MICROBEAM ANALYSIS SOCIETY  
AUSTRALIAN MICROSCOPY AND MICROANALYSIS SOCIETY  
PORTUGUESE SOCIETY FOR MICROSCOPY

PUBLISHED IN AFFILIATION WITH

ROYAL MICROSCOPICAL SOCIETY  
GERMAN SOCIETY FOR ELECTRON MICROSCOPY  
BELGIAN SOCIETY FOR MICROSCOPY  
MICROSCOPY SOCIETY OF SOUTHERN AFRICA

**Editor in Chief**  
**Editor, Biological Applications**  
Robert L. Price  
Cell and Developmental Biology and  
Anatomy  
University of South Carolina  
Columbia, SC 29209  
e-mail: Bob.Price@uscmed.sc.edu

**Editor, Biological Applications**  
Heide Schatten  
Veterinary Pathobiology  
University of Missouri-Columbia  
Columbia, Missouri 65211-5030  
e-mail: schattenh@missouri.edu

**Special Issues and Reviews Editor**  
Jay Jerome  
Vanderbilt University Medical Center  
Nashville, TN 37232  
e-mail: jay.jerome@vanderbilt.edu

**Editor, Materials Applications**  
David J. Smith  
Department of Physics  
School of Materials  
Arizona State University  
Tempe, Arizona 85287-1504  
e-mail: david.smith@asu.edu

**Editor, Microanalysis**  
John Mansfield  
Electron Microbeam Analysis Lab  
North Campus, 417 SRB  
University of Michigan  
Ann Arbor, MI 48109-2143  
e-mail: jfmjfm@umich.edu

**Book Review Editor**  
Cynthia S. Goldsmith  
Centers for Disease Control  
Atlanta, GA 30333  
e-mail: csg1@cdc.gov

**Editor, Scanning Probe  
Microscopies**  
David Bell  
School of Engineering & Applied  
Sciences  
Center for Nanoscale Systems  
Harvard University  
Cambridge, MA 02138  
e-mail: dcb@seas.harvard.edu

**Editor, Correlative and Emerging  
Microscopy Applications**  
Vinayak P. Dravid  
Materials Science and Engineering  
Northwestern University  
Evanston, Illinois 60208-3105  
e-mail: v-dravid@northwestern.edu

**M&M Program Guide Editor**  
Richard E. Edelmann  
Miami University  
Oxford, OH 45056  
e-mail: edelmare@muohio.edu

**Editor, Atom Probe**  
Thomas Kelly  
Cameca Instruments, Inc.  
A Business Unit of AMETEK, Inc.  
Madison, WI 53711-4951  
e-mail: Thomas.Kelly@ametec.com

**Editor, Plant Biology Applications**  
Rosemary White  
CSIRO Plant Industry  
Canberra, ACT 2601, Australia  
e-mail: rosemary.white@csiro.au

**Proceedings Editor**  
John Shields  
University of Georgia  
Athens, GA 30602  
e-mail: jpshield@uga.edu

## Editorial Board

Ralph Albrecht	<i>University of Wisconsin, Madison, Wisconsin</i>
Barry Carter	<i>University of Connecticut, Storrs, Connecticut</i>
Wah Chiu	<i>Baylor College of Medicine, Houston, Texas</i>
Niels de Jonge	<i>INM Institute for New Materials, Saarbrücken, Germany</i>
Alberto Diaspro	<i>University of Genoa, Italy</i>
Elizabeth Dickey	<i>Pennsylvania State University, University Park, Pennsylvania</i>
Alwyn Eades	<i>Lehigh University, Bethlehem, Pennsylvania</i>
Mark Ellisman	<i>University of California at San Diego, San Diego, California</i>
Pratibha Gai	<i>University of York, United Kingdom</i>
Marija Gajdardziska-Josifovska	<i>University of Wisconsin-Milwaukee, Milwaukee, Wisconsin</i>
Dale Johnson	<i>University of South Florida, Tampa, Florida</i>
Paul Kotula	<i>Sandia National Labs, Albuquerque, New Mexico</i>
William Landis	<i>University of Akron, Akron, Ohio</i>
Eric Lifshin	<i>SUNY at Albany, Albany, New York</i>
Charles Lyman	<i>Lehigh University, Bethlehem, Pennsylvania</i>
Dale Newbury	<i>National Institute of Standards and Technology, Gaithersburg, Maryland</i>
Jean-Paul Revel	<i>California Institute of Technology, Pasadena, California</i>
Conly Rieder	<i>Wadsworth Center, Albany, New York</i>
John Silcox	<i>Cornell University, Ithaca, New York</i>
Nestor Zaluzec	<i>Argonne National Laboratory, Argonne, Illinois</i>

## Editorial Board Representatives from Affiliated Societies

Ian Anderson	<i>NIST, Gaithersburg, Maryland (MAS)</i>
Gautam Kumar Dey	<i>Bhabha Atomic Research Centre (EMSI)</i>
Gema Gonzalez	<i>Venezuelan Institute for Scientific Investigation (Venezuela)</i>
Michael Robertson	<i>Acadia University, Wolfville, Nova Scotia (Canada)</i>
Brendan Griffin	<i>University of Western Australia (AMMS)</i>
Guillermo Solorzano	<i>Pontificia Universidade Catolica, Rio de Janeiro (Brazil)</i>
Clive Walker	<i>Institute for Transuranium Elements, Karlsruhe (EMAS)</i>
Miguel Yacamán	<i>Mexico Institute for Nuclear Research (Mexico)</i>
Henrique Almeida	<i>Universidade do Porto (Portugal)</i>

## Founding Editor

Jean-Paul Revel	<i>California Institute of Technology, Pasadena, California</i>
-----------------	---


## Previous Editors-in-Chief

Dale Johnson	<i>University of South Florida, Tampa, Florida</i>
Charles Lyman	<i>Lehigh University, Bethlehem, Pennsylvania</i>

This journal is part of the **Cambridge Journals Online** service. Access to online tables of contents and article abstracts is available to all researchers at no cost. Access to full-text articles online is provided to those with online subscription. Online subscriptions must be activated. Once your subscription is activated, free access to past, present, and forthcoming articles is available at:

**Microscopy and Microanalysis website: [journals.cambridge.org/MAM](http://journals.cambridge.org/MAM).**

Instructions for authors submitting manuscripts may be found at [journals.cambridge.org/MAM](http://journals.cambridge.org/MAM). Select "Further Information" then select "Instructions for Contributors." An abbreviated version of these instructions will be published in the first issue (February) of each volume.

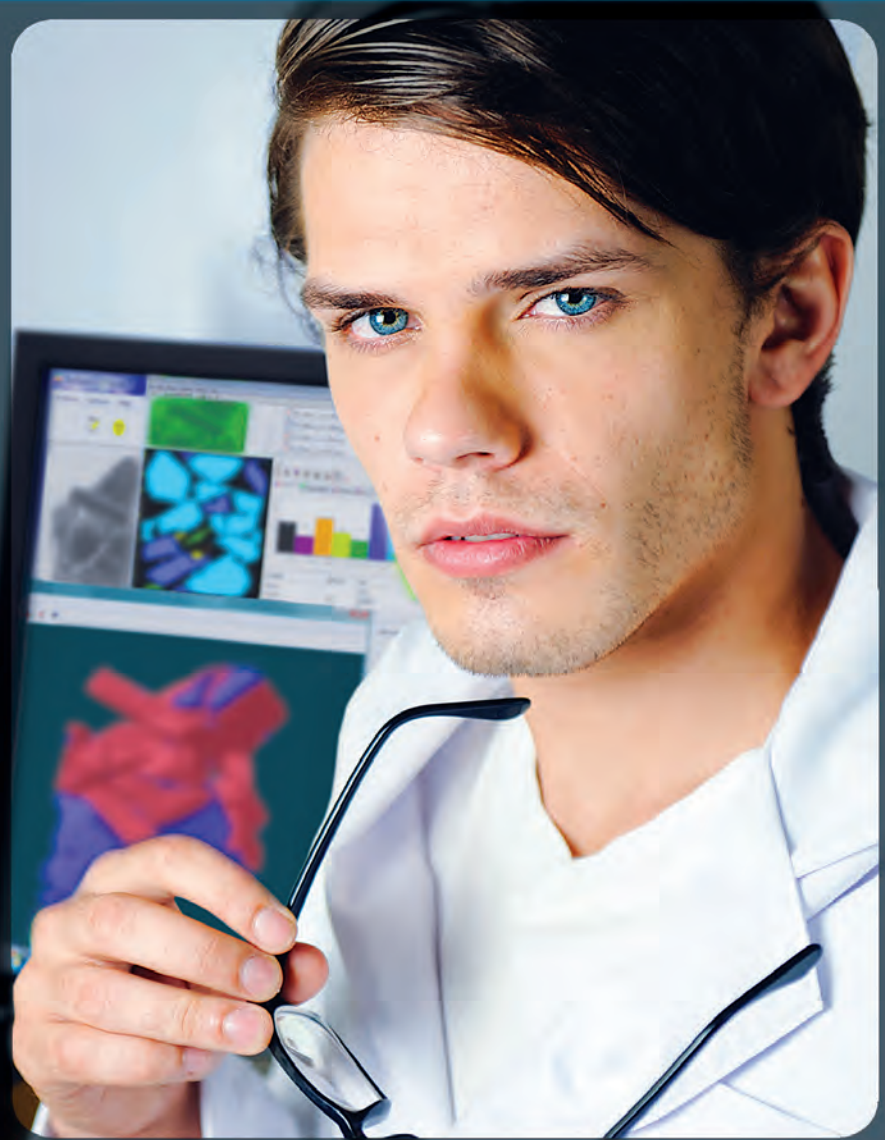

Bruker microCT formerly known as SkyScan develops and produces wide range of high-end microtomography instruments for life science, material research and *in-vivo* preclinical studies



free QR-reader app is available in the AppStore

- Micro-computed tomography or "micro-CT" is X-ray imaging in 3D, by the same method used in hospital CT (or "CAT") scans, but on a small scale with massively increased resolution.
- It really represents true 3D microscopy, where very fine scale internal structure of objects is imaged non-destructively.
- No sample preparation, no staining, no coating, no thin slicing.
- A single scan will image complete internal 3D structure of your object,
- Plus you get your intact sample back at the end!

Innovation with Integrity

[bruker-microct.com](http://bruker-microct.com)

microtomography

*Microscopy and Microanalysis* publishes original research papers dealing with a broad range of topics in microscopy and microanalysis. These include articles describing new techniques or instrumentation and their applications, as well as papers in which established methods of microscopy or microanalysis are applied to important problems in the fields of biology or materials science. Microscopy and microanalysis are defined here in a broad sense, and include all current and developing approaches to the imaging and analysis of microstructure. The criteria for acceptance of manuscripts are the originality and significance of the research, the quality of the microscopy or microanalysis involved, and the interest for our readership.

Four types of communications are published in the Journal. **Regular Articles** are of substantial length and describe the findings of an original research project that satisfies the aims and scope of the Journal, described above. **Review Articles** summarize the current status of an important area within the aims and scope of the Journal. **Letters to the Editor** usually contain comments on recent articles that have appeared in the Journal. **Book Reviews** are also published, but these are solicited only through the Book Review Editor.

### Instructions for Contributors

Instructions for authors contributing manuscripts may be found at <http://mc.manuscriptcentral.com/mam> under "Resources: Instructions and Forms." Authors may also visit [http://www.journals.cambridge.org/jid\\_MAM](http://www.journals.cambridge.org/jid_MAM), select "Further Information," and then select "Instructions for Contributors." An abbreviated version of these instructions will be published in the first issue (February) of each volume.

### Copyright Information

Submission of a manuscript implies: that the work described has not been published before (except in the form of an abstract or as part of a published lecture, review, or thesis); that it is not under consideration for publication elsewhere; that its publication has been approved by all coauthors, if any, as well as by the responsible authorities at the institute where the work has been carried out; that, if and when the manuscript is accepted for publication, the authors agree to automatic transfer of the copyright to the Microscopy Society of America; that the manuscript will not be published elsewhere in any language without the consent of the copyright holders; and that written permission of the copyright holder is obtained by the authors for material used from other copyrighted sources.

All articles published in this journal are protected by copyright, which covers the exclusive rights to reproduce and distribute the article (e.g., as offprints), as well as all translation rights. No material published in this journal may be reproduced photographically or stored on microfilm, in electronic data bases, video disks, etc., without first obtaining written permission from the publisher.

The use of general descriptive names, trade names, trademarks, etc., in this publication, even if not specifically identified, does not imply that these names lack protection by the relevant laws and regulation.

Authorization to photocopy items for internal or personal use, or the internal or personal use of specific clients, is granted by Cambridge University Press, provided that the appropriate fee is paid directly to Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, USA (Tel: (508) 750-8400), stating the ISSN (1431-9276), the volume, and the first and last page numbers of each article copied. The copyright owner's consent does not include copying for general distribution, promotion, new works, or resale. In these cases, specific written permission must first be obtained from the publisher.

### Disclaimer

The Microscopy Society of America, the other societies stated, and Cambridge University Press cannot be held responsible for errors or for any consequences arising from the use of the information contained in this journal. The appearance of scientific reports and/or workshops, or any other material in *Microscopy and Microanalysis* does not constitute an endorsement or approval by The Microscopy Society of America of the findings, data, conclusions, recommendations, procedures, results, or any other aspect of the content of such articles. The appearance of advertising in *Microscopy and Microanalysis* does not constitute an endorsement or approval by The Microscopy Society of America of the quality or value of the products advertised or any of

the claims, data, conclusions, recommendations, procedures, results, or any other information included in the advertisements.

While the advice and information in this journal is believed to be true and accurate at the date of its going to press, neither the authors, the editors, nor the publisher can accept any legal responsibility for any errors or omissions that may be made.

### Subscription Information

*Microscopy and Microanalysis* is published bimonthly in February, April, June, August, October, and December by Cambridge University Press. Two supplements (*Expo* and *Proceedings*) are published in June and August.

**Society Rates:** Members of the Microscopy Society of America should contact the MSA Business Office for all subscription inquiries: Microscopy Society of America, Hachero Hill, Inc., 11260 Roger Bacon Drive, Suite 402, Reston, VA 20190, Tel.: (703) 964-1240, Ext. 14, E-mail: [nicoleguy@mindspring.com](mailto:nicoleguy@mindspring.com), URL: [www.msa.microscopy.org](http://www.msa.microscopy.org). Members of other affiliated societies should contact their respective society business offices for all subscription inquiries.

**Subscription Rates:** Institutions print and electronic: US \$957.00 in the USA, Canada, and Mexico; UK £577.00 + VAT elsewhere. Institutions online only: US \$790.00 in the USA, Canada, and Mexico; UK £478.00 + VAT elsewhere. Institutions print only: US \$863.00 in the USA, Canada, and Mexico; UK £520.00 + VAT elsewhere. Individuals print and online: US \$359.00 in the USA, Canada, and Mexico; UK £218.00 + VAT elsewhere. Prices include postage and insurance.

**USA, Canada, and Mexico:** Subscribers in the USA, Canada, and Mexico should send their orders, with payment in US dollars or the equivalent value in Canadian dollars, to: Cambridge University Press, Customer Services Department (Journals), 100 Brook Hill Drive, West Nyack, NY 10994-2133, USA. Tel: (845) 353-7500. Fax: (845) 353-4141. Orders may be phoned direct (toll free): (800) 872-7423. E-mail: [journals\\_subscriptions@cup.org](mailto:journals_subscriptions@cup.org).

**Outside North America:** Subscribers elsewhere should send their orders, with payment in sterling, to: Customer Services Department (Journals), Cambridge University Press, The Edinburgh Building, Shaftesbury Road, Cambridge, CB2 8RU, UK. Tel: +44 (0)1223 326070. Fax: +44 (0)1223 325150. E-mail: [journals@cambridge.org](mailto:journals@cambridge.org)

**Change of address:** Allow six weeks for all changes to become effective. All communications should include both old and new addresses (with postal codes) and should be accompanied by a mailing label from a recent issue. Society members should contact their respective society business offices to inform them of address changes.

**Microform editions are available from:** University Microfilms International, 300 North Zeeb Road, Ann Arbor, MI 48106, USA.

### Editorial Office

Robert L. Price, Editor in Chief, Department of Cell and Developmental Biology and Anatomy, School of Medicine, University of South Carolina, 6439 Garner's Ferry Road, Bldg. 1 B-60, Columbia, SC 29209, USA; Tel: (803) 216-3824; Fax: (803) 733-3212; E-mail: [Bob.Price@uscmed.sc.edu](mailto:Bob.Price@uscmed.sc.edu).

### Office of Publication

Cambridge University Press, 32 Avenue of the Americas, New York, NY 10013-2473, USA; Tel: (212) 337-5000; Fax: (212) 337-5959.

### Advertising Sales & Production

M.J. Mrvica Associates, Inc., 2 West Taunton Avenue, Berlin, NJ 08009, USA; Tel: (856) 768-9360; Fax: (856) 753-0064.

© 2013 by Microscopy Society of America. Printed in the United States on acid-free paper. Periodicals postage paid at New York, NY, and additional mailing offices. Return postage guaranteed. Postmaster: Send address changes in the U.S.A. and Canada to *Microscopy and Microanalysis*, Subscription Department, Cambridge University Press, 100 Brook Hill Drive, West Nyack, NY 10994-2133.

# The SPI Supplies Family of Instruments



Excellence in sample preparation  
just a click away... [2spi.com](http://2spi.com)

Your results will never be better than your sample preparation. See how SPI Supplies can help you deliver the highest quality results for all your SEM/EDS, TEM and FESEM applications.

1. **Osmium Plasma Coaters**  
for FESEM Applications
2. **SPI-MODULE™**  
Sputter/Carbon Coater Module
3. **Gentle Mill™**  
Ion Milling System
4. **Plasma Prep™ III** Solid State  
Plasma Cleaner for cleaning TEM holders

5. **Plasma Prep™ X**  
Parallel Plate Plasma Etcher
6. **Plasma Prep™ III** Plasma Etcher  
with PPIII Process Controller
7. **Vacu Prep™ II**  
Turbo Pump Evaporation System
8. **SPI-DRY™**  
Critical Point Dryer
9. **Precision Spin Coater**  
Spin coater



SPI Supplies Division of **STRUCTURE PROBE, Inc.**

P.O. Box 656 • West Chester, PA 19381-0656 USA  
Phone: 1-610-436-5400 • 1-800-2424-SPI (USA and Canada) • Fax: 1-610-436-5755 • [2spi.com](http://2spi.com) • E-mail: [sales@2spi.com](mailto:sales@2spi.com)





Cooling Stages  
Recirculating Heaters and Chillers  
Sputter Coaters  
SEM/TEM Carbon Coaters  
Vacuum Evaporators  
Glow Discharge Systems  
RF Plasma Etchers/  
Plasma Reactors  
Critical Point Dryers  
Freeze Dryers  
Cryo-SEM Preparation Systems  
Vacuum Pumps & Accessories  
Evaporation Supplies  
**and more...**

## well equipped...

Electron Microscopy Sciences is pleased to announce our new full line catalog, your comprehensive source for high-end Vacuum Equipment. EMS is committed to providing the highest quality products along with competitive pricing, prompt delivery and outstanding customer service.



## and more...

Not just Vacuum Equipment, EMS also offers:

Laboratory Microwave Ovens • Automated Tissue Processors • Oscillating Tissue Slicers • Vibrating Microtomes • Rapid Immersion Freezers • Tissue Choppers • Desiccators and Desiccants • Centrifuges, Tubes, and Racks • Stirrers, Stirring Hotplates, and Digital Hotplates • Stirring Bars, Stirring Rods, and Hand Mixers • Vortex Mixers, Microplate Mixers, and Magnetic Stirrers • Tissue Rotators, Mixer Vortexes, and Rotator/Rockers • Dri Baths • Oven/Incubators • Cooling Chambers • Ultraviolet Lamps • Lab Jacks

For catalog requests, please visit our website at [www.emsdiasum.com](http://www.emsdiasum.com)



**Electron  
Microscopy  
Sciences**

Electron Microscopy Sciences  
P.O. Box 550 • 1560 Industry Rd. • Hatfield, Pa 19440  
Tel: (215) 412-8400 • Fax: (215) 412-8450  
email: [sgkck@aol.com](mailto:sgkck@aol.com) • [www.emsdiasum.com](http://www.emsdiasum.com)




# Microscopy AND Microanalysis

An International Journal for the Biological and Physical Sciences

Volume 19, Number 1  
February 2013

## SOFTWARE, TECHNIQUES AND EQUIPMENT DEVELOPMENT

- EMEN2: An Object Oriented Database and Electronic Lab Notebook 1  
*Ian Rees, Ed Langley, Wah Chiu, and Steven J. Ludtke*
- Variable Phase Bright-Field Contrast—An Alternative Illumination Technique  
for Improved Imaging in Transparent Specimens 11  
*Timm Piper and Jörg Piper*
- Laboratory-Based Cryogenic Soft X-Ray Tomography with Correlative  
Cryo-Light and Electron Microscopy 22  
*David B. Carlson, Jeff Gelb, Vadim Palshin, and James E. Evans*
- Novel Method for Controlled Wetting of Materials in the Environmental  
Scanning Electron Microscope 30  
*Anna Jansson, Alexandra Nafari, Anke Sanz-Velasco, Krister Svensson,  
Stefan Gustafsson, Anne-Marie Hermansson, and Eva Olsson*
- Low-Dosage Maximum-A-Posteriori Focusing and Stigmatism 38  
*Jonas Binding, Shawn Mikula, and Winfried Denk*
- Analysis of Biologically-Derived Small Particles—Searching for  
Geometry Correction Factors Using Monte Carlo Simulation 56  
*Grzegorz Tylko*
- A Standards-Based Method for Compositional Analysis by Energy  
Dispersive X-Ray Spectrometry Using Multivariate Statistical Analysis:  
Application to Multicomponent Alloys 66  
*Monika Rathi, S.P. Ahrenkiel, J.J. Carapella, and M.W. Wanlass*
- A Method for Producing Site-Specific TEM Specimens from Low Contrast  
Materials with Nanometer Precision 73  
*Henrik Pettersson, Samira Nik, Jonathan Weidow, and Eva Olsson*
- FIB Preparation of a NiO Wedge-Lamella and STEM X-Ray Microanalysis  
for the Determination of the Experimental  $k(\text{O-Ni})$  Cliff-Lorimer Coefficient 79  
*Aldo Armigliato, Stefano Frabboni, Gian Carlo Gazzadi, and Rodolfo Rosa*
- Three-Dimensional Semiconductor Device Investigation Using Focused Ion Beam  
and Scanning Electron Microscopy Imaging (FIB/SEM Tomography) 85  
*K. Lepinay and F. Lorut*
- The Influence of the Sample Thickness on the Lateral and Axial Resolution  
of Aberration-Corrected Scanning Transmission Electron Microscopy 93  
*Ranjan Ramachandra, Hendrix Demers, and Niels de Jonge*

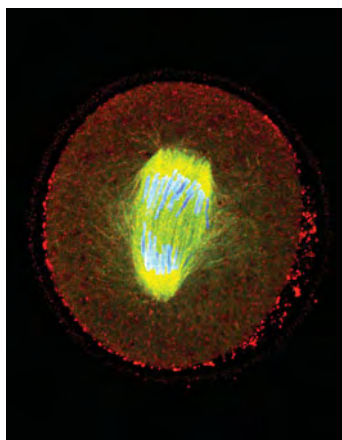

**On the Cover:** Expression of ERK8 during Anaphase I of mouse oocyte meiosis. For further information see Yang et al. pp. 190–200.

**Microscopy and Microanalysis website:** <http://www.journals.cambridge.org/MAM>  
Indexed in Chemical Abstracts, Current Contents, BIOSIS, and MEDLINE (PubMed)

## MATERIALS APPLICATIONS

- Microstructural and Chemical Characterization of Ordered Structure in Yttrium Doped Ceria 102  
*Pengfei Yan, Toshiyuki Mori, Yuanyuan Wu, Zhimin Li, Graeme John Auchterlonie, Jin Zou, and John Drennan*
- Grain Boundary Character Distribution of Nanocrystalline Cu Thin Films Using Stereological Analysis of Transmission Electron Microscope Orientation Maps 111  
*A.D. Darbal, K.J. Ganesh, X. Liu, S.-B. Lee, J. Ledonne, T. Sun, B. Yao, A.P. Warren, G.S. Rohrer, A.D. Rollett, P.J. Ferreira, K.R. Coffey, and K. Barmak*
- Electron Microscopy Characterization of Ni-Cr-B-Si-C Laser Deposited Coatings 120  
*I. Hemmati, J.C. Rao, V. Ocelik, and J.Th.M. De Hosson*
- Investigation of Organic Matter Entrapped in Synthetic Carbonates—A Multimethod Approach 132  
*Emilie Chalmin, Yves Perrette, Bernard Fanget, and Jean Susini*

## BIOLOGICAL APPLICATIONS

- Examining Protein Crystallization Using Scanning Electron Microscopy 145  
*Kathryn Gomery, Elaine C. Humphrey, and Rodney Herring*
- A High-Content, Live-Cell, and Real-Time Approach to the Quantitation of Ligand Induced  $\beta$ -Arrestin2 and Class A/Class B GPCR Mobilization 150  
*Anthony P. Leonard, Kathryn M. Appleton, Louis M. Luttrell, and Yuri K. Peterson*
- Ma-PbFRET: Multiple Acceptors FRET Measurement Based on Partial Acceptor Photobleaching 171  
*Huaina Yu, Jianwei Zhang, Huali Li, and Tongsheng Chen*
- Automated Podosome Identification and Characterization in Fluorescence Microscopy Images 180  
*Marjolein B.M. Meddens, Bernd Rieger, Carl G. Figdor, Alessandra Cambi, and Koen van den Dries*
- The Distribution and Possible Role of ERK8 in Mouse Oocyte Meiotic Maturation and Early Embryo Cleavage 190  
*Shang-Wu Yang, Hao Huang, Chen Gao, Lei Chen, Shu-Tao Qi, Fei Lin, Jian-Xin Wang, Yi Hou, Fu-Qi Xing, and Qing-Yuan Sun*
- Intravital Confocal and Two-Photon Imaging of Dual-Color Cells and Extracellular Matrix Mimics 201  
*Ufuk Bal, Volker Andresen, Brenda Baggett, and Urs Utzinger*
- Characterization of Polymeric Microcapsules Containing a Low Molecular Weight Peptide for Controlled Release 213  
*Keith Moore, Jennifer Amos, Jeffrey Davis, Robert Gourdie, and Jay D. Potts*
- Short-Term Response of Mitomycin C on the Human Rectus Muscle Following Strabismus Surgery: Histological, Ultrastructural, and Biomechanical Evaluation 227  
*Samjin Choi, Youjin Cheong, Jae-Ho Shin, Kyung A Kim, Jae Beum Bang, Kyung-Hyun Jin, and Hun-Kuk Park*
- The Expression of Alkaline Phosphatase, Osteopontin, Osteocalcin, and Chondroitin Sulfate during Pectoral Fin Regeneration in *Carassius auratus gibelio*: A Combined Histochemical and Immunohistochemical Study 233  
*Simona Stavri and Otilia Zarnescu*
- Transmission Electron Microscopy, Fluorescence Microscopy, and Confocal Raman Microscopic Analysis of Ultrastructural and Compositional Heterogeneity of *Cornus alba* L. Wood Cell Wall 243  
*Jianfeng Ma, Zhe Ji, Xia Zhou, Zhiheng Zhang, and Feng Xu*
- Effects of *Mesua ferrea* Leaf and Fruit Extracts on Growth and Morphology of *Staphylococcus aureus* 254  
*Claira Arul Aruldass, Mani Maran Marimuthu, Surash Ramanathan, Sharif Mahsufi Mansor, and Vikneswaran Murugaiyah*

The moment "I think" becomes "I know".  
**This is the moment we work for.**


// TECHNOLOGY  
MADE BY CARL ZEISS

## High Definition Imaging from Carl Zeiss

$\Sigma$ IGMA HD introduces faster and higher definition imaging to analytical field emission scanning electron microscopy. Available in both high vacuum and variable pressure modes,  $\Sigma$ IGMA HD allows for imaging structures as small as 1 nm, and the GEMINI column provides superb low voltage stability.

$\Sigma$ IGMA HD has been optimized for the latest analytical detectors with a total of fifteen ports including two dedicated EDS ports mounted diametrically opposite, a third off-axis EDS port, plus WDS and EBSD ports for maximum throughput.  $\Sigma$ IGMA HD is highly suited for multipurpose facilities requiring high resolution without compromising flexibility.

Contact Carl Zeiss or visit our website to request more information, including how you can collect data for your next grant.

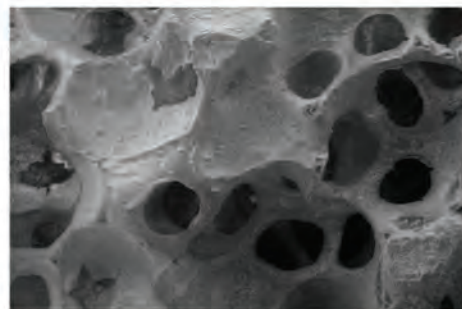

**Carl Zeiss Microscopy, LLC**

[micro@zeiss.com](mailto:micro@zeiss.com)

[www.zeiss.com/sigma](http://www.zeiss.com/sigma)

<https://doi.org/10.1017/S1431927613000068> Published online by Cambridge University Press



We make it visible.

# Are you pushing the envelope?



**The LYRA GM FIB-SEM workstation  
is the most recent FIB-SEM workstation offering from TESCAN.  
Designed for simultaneous EDS, WDS, EBSD and TOF SIMS while milling.**

**Contact us and find out why  
more and more researchers are choosing TESCAN.**

- \*Thermionic Scanning Electron Microscopes
- \*Field Emission Scanning Electron Microscopes
- \*FIB-SEM Workstations
- \*FIB-SEM Time of Flight Integration
- \*Plasma FIB-SEM Workstations



**[www.tescan.com](http://www.tescan.com)  
[www.tescan-usa.com](http://www.tescan-usa.com)**

**TESCAN USA, 508 Thomson Park Drive, Cranberry Twp., PA 16066, Tel: 724-772-7433, Email: [info@tescan-usa.com](mailto:info@tescan-usa.com)**